

A Workflow for Probabilistic Calibration of Models of Left Atrial Electrophysiology

Sam Coveney¹, Cesare Corrado³, Caroline Roney⁴, Richard D Wilkinson⁵, Jeremy E Oakley², Steven A Niederer³, Richard H Clayton²

¹ University of Leeds, Leeds, UK

² University of Sheffield, Sheffield, UK

³ King's College London, London, UK

⁴ Queen Mary University of London, London, UK

⁵ University of Nottingham, Nottingham, UK

Abstract

Atrial fibrillation is an increasingly common condition. Computational models that describe left atrial electrophysiology have the potential to be used to guide interventions such as catheter ablation. Calibration of these models to faithfully represent left atrial structure and function in a particular patient is challenging because electrophysiology observations obtained in the clinical setting are typically sparse and noisy, and can be difficult to register to a mesh obtained from imaging.

Probabilistic approaches show promise as a way to obtain personalised models while taking account of noise, sparseness, and uncertainty. We have developed a workflow in which parameter fields are represented as Gaussian processes, and the posterior distribution is inferred using MCMC. Our workflow has been tested using synthetic data, generated from simulations where the spatial variation in model parameters is known, and we have shown that both features and parameters can be recovered from simulated sparse measurements.

1. Introduction

Atrial fibrillation (AF) is an increasingly prevalent arrhythmia, and the left atrium (LA) is often the main source of fibrillatory activity [1]. Persistent AF can be treated by catheter ablation, and treatment guidance using personalised models offers promise for streamlining these procedures and improving outcomes for patients [2].

The main components of a personalised LA model are a mesh constructed from imaging data, and a calibrated model of LA electrophysiology. Model calibration is challenging because the measurements available in the routine clinical setting are far from sufficient to fully calibrate biophysically detailed models. In this paper we describe a

workflow that has been developed to address these challenges using a probabilistic approach [3–6]. In this paper, we review the different components of this workflow, with an emphasis on conduction velocity (CV).

2. Background

The overall goal is to be able to calibrate an electrophysiology model so that model parameters that define local CV and action potential (APD), as well as their restitution, are determined at each mesh vertex. The starting point of the workflow is a mesh representing the left atrium (LA), and bipolar electrograms recorded at different locations within the LA and at different pacing cycle lengths. From these observations, we estimate local activation time (LAT) at the electrode locations.

Bipolar electrograms are routinely used in the clinical setting because they are less susceptible to far-field effects than unipolar electrograms, but there is no generally accepted way to assign LAT to these signals [7]. We therefore developed a modified centre-of-mass method to identify LAT [3].

The second step is to interpolate LAT across the LA mesh, taking into account uncertainties arising from both the identification of LAT from the bipolar signal and registration of the electrode co-ordinates with the mesh. Interpolation of LAT across the LA mesh involves taking a set of uncertain measurements LAT_{mesh} obtained from clinical bipolar electrograms at a subset of mesh vertices, and using this information to interpolate LAT over the entire mesh. In this approach the noisy observations of LAT ($y_i \equiv LAT_{mesh}$) at a particular location x_i are modelled as

$$y_i = f(x_i) + \epsilon_i, \quad (1)$$

where ϵ_i is normally distributed noise at location x_i with

mean of zero and standard deviation σ^2 . The standard deviation of the error in each observation can be different i.e. heteroscedastic noise, or the same i.e. homoscedastic. It is possible to model $f(x_i)$ using a variety of methods [8], but we chose to model it as a Gaussian process (GP).

Having obtained a probabilistic interpolation of LAT, the third step is to calculate the inverse of the gradient in LAT, to obtain an uncertain estimate of CV at each mesh vertex. The fourth and final step is to use these estimates to calibrate the electrophysiology model. A key challenge at this stage is that there is not a simple mapping between these features and model parameters.

In the next section we describe the third and fourth step in more detail

3. Uncertain CV interpolation

Standard types of covariance function, which use Euclidean distances between pairs of mesh vertices, are not suitable since the Euclidean distance does not reflect the distance travelled by an activation wave over the curved LA mesh. Neither is it possible to use simple geodesic distances over the mesh because the resulting covariance matrix is not positive semi-definite. We therefore initially used an approach based on Gaussian Markov random fields (GMRF), where the covariance function (more specifically the precision matrix) is approximated as a solution to a stochastic partial differential equation solved on the mesh [9]. The GMRF approach was successful, not only in providing interpolation of LAT but also in enabling interpolation of uncertain LAT fields across different S1S2 pacing intervals [3].

The GMRF approach could be used to obtain a posterior mean of LAT, and by calculating the inverse of the gradient of this field we could obtain a posterior mean for CV. However it was difficult to map uncertainty in LAT to uncertainty in CV by stochastic sampling of the posterior LAT. The posterior LAT samples were not smooth because the type of Matérn function used in the GMRF method covariance function was constrained to take a form that is not differentiable, and thus could not be used to calculate CV. An alternative, and faster, method was therefore devised to solve this problem [4] based on [10].

Key to this Gaussian process manifold interpolation (GPMI) approach is an alternative way to construct the GP covariance kernel as a basis function expansion. The basis functions are eigenfunctions corresponding to the smallest K eigenvalues of the Laplacian operator on the mesh, combined with a spectral density that takes a form based on a covariance function – see equations 2.5 and 2.6 of [4] for details. These functional forms take account of the mesh geometry and topology, can be calculated on the atrial mesh using standard approaches, and need only to be calculated once.

A further benefit of the GPMI approach is that the gradient of a GP is also a GP because gradient is a linear operator. Thus it is possible to obtain the posterior mean and the variance of *gradients* in LAT, as well as LAT itself (see equations 2.9 and 2.10 in [4]). The posterior mean of CV is then the inverse of the posterior mean of the gradient of LAT. Uncertainty in CV cannot be determined directly from the posterior variance in gradient of LAT because neither inverse nor magnitude are linear operators. Instead, the posterior CV distribution is estimated by sampling the posterior gradient in LAT 2000 times, and inverting each sample. To obtain the multivariate posterior distribution of CV, one would need to sample the gradient LAT posterior many times, and calculate CV from each sample.

A Python implementation of the GPMI method is available at <https://zenodo.org/badge/latestdoi/10.5281/zenodo.239559025>.

4. Step 4 - EP model calibration

Having obtained probabilistic interpolation of LAT and CV, the next step was to use this information for calibration of an EP model. The goal was to produce uncertain parameter fields from which samples could be drawn and simulations run that capture the uncertainties in both the measurements and the calibration process. Identifiability of parameters remains a serious and possibly intractable problem for biophysically detailed cell models [11], and so we have started with a simplified and phenomenological model with 5 parameters that nevertheless reproduces key dynamic action potential features [12].

Calibration of this model to observable data required a mapping between CV and the model parameters. A key dynamic feature of cardiac electrophysiology is restitution, and understanding the relationship between tissue restitution and model parameters was an important component of calibration. To address this problem, we generated data from simulations in a tissue strip to learn the relationship between CV and a reparameterisation of the model parameters. We decomposed a set of restitution curves obtained from strip simulations using principal component analysis (PCA), finding via a sensitivity analysis that the curves could be represented either 2 or 3 principal components [5]. We then built surrogate models of these components, which provided a link between the model parameters and the restitution curves. Model parameters could then be estimated using maximum a posteriori (MAP) estimation, and the distribution of parameters estimated by Markov Chain Monte Carlo (MCMC) sampling.

The next challenge has been to extend model calibration to the left atrial mesh [6]. This approach combines the GPMI method [4] and surrogate models of restitution [5]. There are two important assumptions. First, we assume that uncertainty in CV at each mesh vertex is Gaussian, and

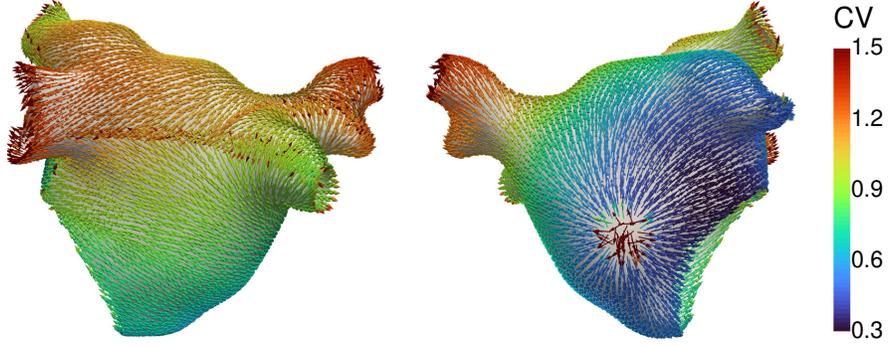


Figure 1. Ground truth CV (in m/s) from simulation with pacing at the coronary sinus.

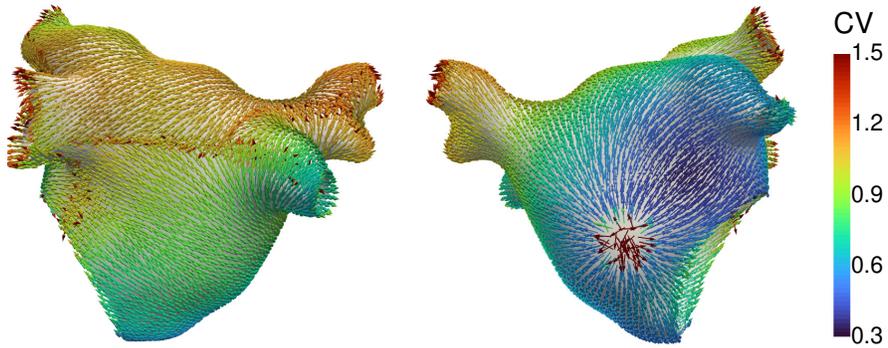


Figure 2. Predicted CV (in m/s) obtained by running a simulation using parameters inferred via “observations” of CV.

this can be estimated from interquartile ranges. Second, we treat the CV at each mesh vertex as independent, whereas the overall CV on the mesh is correlated.

GPMI is used to represent each model parameter θ as a spatially correlated random field extending over the LA mesh at locations \mathbf{x}

$$\theta(\mathbf{x}) = m + \alpha \sum_{k=1}^K \eta_k \sqrt{S(\sqrt{\lambda_k}, \rho)} \phi_k(\mathbf{x}) \quad (2)$$

$$\eta_k \sim \mathcal{N}(0, 1). \quad (3)$$

Here the mean m , amplitude α and lengthscale ρ are hyperparameters that are learned, conditional on CV obtained at locations where LAT was observed, through Bayesian inference; S is a spectral density determined from the covariance kernel; λ_k and ϕ_k are the K eigenvalues and eigenfunctions obtained from solving the Laplacian on the mesh. The distributions of parameters are then obtained conditional on observations, by MCMC. We use the first 256 eigenvalues for interpolation of LAT, but for MCMC we use 64 to reduce the computational burden. This is

a very similar model to that used for interpolation, but is more flexible in that m , α , and lengthscale, can all be given priors, and the likelihood on the observations can be anything we choose.

In [6] we concentrate on inference for the parameters that determine ERP and ERP restitution. We show that we can use a small number of synthetic observations of ERP at different pacing cycle lengths obtained from a simulation to retrieve estimates of the model parameters used in the simulation. In Figures 1 and 2 we show that the spatial heterogeneity in CV can also be recovered.

Figure 1 shows CV obtained from a simulation with pacing at the coronary sinus, with heterogeneity in model parameter producing heterogeneity in CV. A separate simulation was then performed, using the same model parameters and with pacing at the right pulmonary vein. Observations of LAT, with added Gaussian noise with standard deviation 1 ms and at a set of discrete locations were then used to infer CV across the mesh, and this information was used to estimate the recovered model parameters. This is done with MCMC, using a Gaussian likelihood for CV ‘observations’ and the prior of equations (4)-(4). Figure 2 shows the CV obtained from a simulation with the recovered parameters and pacing at the coronary sinus.

5. Discussion and outlook

This work has addressed the problem of probabilistic interpolation and model calibration on a manifold. We have shown that it is possible to interpolate clinical observations and to recover model parameters used to produce synthetic observations. Nevertheless, several challenges and limitations remain.

Other approaches have been developed (for example [13]), but these can be computationally intensive.

The identification and uniqueness of model parameters is a serious and fundamental difficulty, especially for biophysically detailed models. In the face of this challenge, it is reasonable to develop approaches where model parameters are fixed, or vary spatially in predefined ways. However, with the goal of guiding clinical interventions such as catheter ablation it is important to probe whether calibration is possible.

A related question is whether spatial heterogeneity in model parameters is actually important. A key factor in this discussion is the extent to which spatial heterogeneity in parameters affects the behaviour of re-entry and prediction of ablation targets. It is well known that structure, and especially fibrosis, has an important impact on both of these features. Integration of structural data such as fibrosis maps obtained from imaging, will be an exciting next step in the development of the ideas discussed in this paper.

Acknowledgments

This work was funded by the UK Engineering and Physical Sciences Research Council through grants EP/P010741/1, EP/P01268X/1, and EP/T017899/1.

References

- [1] Krummen DE, Bayer JD, Ho J, Ho G, Smetak MR, Clifton P, Trayanova NA, Narayan SM. Mechanisms of human atrial fibrillation initiation: Clinical and computational studies of repolarization restitution and activation latency. *Circulation Arrhythmia and Electrophysiology* December 2012;5(6):1149–1159.
- [2] Boyle PM, Zghaib T, Zahid S, Ali RL, Deng D, Franceschi WH, Hakim JB, Murphy MJ, Prakosa A, Zimmerman SL, Ashikaga H, Marine JE, Kollandaivelu A, Nazarian S, Spragg DD, Calkins H, Trayanova NA. Computationally guided personalized targeted ablation of persistent atrial fibrillation. *Nature Biomedical Engineering* November 2019; 3(11):870–879.
- [3] Coveney S, Corrado C, Roney C, Wilkinson R, Oakley J, Lindgren F, Williams S, O’Neill MD, Niederer S, Clayton R. Probabilistic Interpolation of Uncertain Local Activation Times on Human Atrial Manifolds. *IEEE Transactions on Biomedical Engineering* 2019;99–109.
- [4] Coveney S, Corrado C, Roney CH, O’Hare D, Williams SE, O’Neill MD, Niederer SA, Clayton RH, Oakley JE, Wilkinson RD. Gaussian process manifold interpolation for probabilistic atrial activation maps and uncertain conduction velocity. *Philosophical Transactions of the Royal Society A Mathematical Physical and Engineering Sciences* June 2020;378(2173):20190345.
- [5] Coveney S, Corrado C, Oakley JE, Wilkinson RD, Niederer SA, Clayton RH. Bayesian Calibration of Electrophysiology Models Using Restitution Curve Emulators. *Frontiers in Physiology* July 2021;12:693015.
- [6] Coveney S, Roney CH, Corrado C, Wilkinson RD, Oakley JE, Niederer SA, Clayton RH. Calibrating cardiac electrophysiology models using latent Gaussian processes on atrial manifolds 2022;.
- [7] Cantwell CD, Roney CH, Ng FS, Siggers JH, Sherwin SJ, Peters NS. Techniques for automated local activation time annotation and conduction velocity estimation in cardiac mapping. *Computers in Biology and Medicine* 2015; 65:229–242.
- [8] Coveney S, Cantwell C, Roney C. Atrial conduction velocity mapping: Clinical tools, algorithms and approaches for understanding the arrhythmogenic substrate. *Medical Biological Engineering Computing* September 2022; 60(9):2463–2478.
- [9] Lindgren F, Rue H, Lindström J. An explicit link between Gaussian fields and Gaussian Markov random fields: The stochastic partial differential equation approach: Link between Gaussian Fields and Gaussian Markov Random Fields. *Journal of the Royal Statistical Society Series B Statistical Methodology* September 2011;73(4):423–498.
- [10] Solin A, Särkkä S. Hilbert space methods for reduced-rank Gaussian process regression. *Statistics and Computing* March 2020;30(2):419–446.
- [11] Whittaker DG, Clerx M, Lei CL, Christini DJ, Mirams GR. Calibration of ionic and cellular cardiac electrophysiology models. *WIREs Systems Biology and Medicine* July 2020; 12(4):e1482.
- [12] Corrado C, Niederer SA. A two-variable model robust to pacemaker behaviour for the dynamics of the cardiac action potential. *Mathematical Biosciences* November 2016; 281:46–54.
- [13] Grandits T, Pezzuto S, Lubrecht JM, Pock T, Plank G, Krause R. PIEMAP: Personalized Inverse Eikonal Model from Cardiac Electro-Anatomical Maps. In Puyol Anton E, Pop M, Sermesant M, Campello V, Lalande A, Lekadir K, Suinesiaputra A, Camara O, Young A (eds.), *Statistical Atlases and Computational Models of the Heart. M&Ms and EMIDEC Challenges*, volume 12592. Cham: Springer International Publishing, 2021; 76–86.

Address for correspondence:

Richard Clayton
Department of Computer Science,
Regent Court, 211 Portobello St,
Sheffield S1 4DP,
United Kingdom.
r.h.clayton@sheffield.ac.uk